

# PhyView Analyzer DC Unbalance Report

PVA: 192.168.221.141  
PSA: 192.168.221.141




PVA Port: 7-2  
PSA Port: 1-2

Date: April 25 2012  
Time: 5:45 PM

PSE: Sample Type-2 PSE Port  
PSE Port: 1



PHY Suite Version: 4.0.12 04-24-12

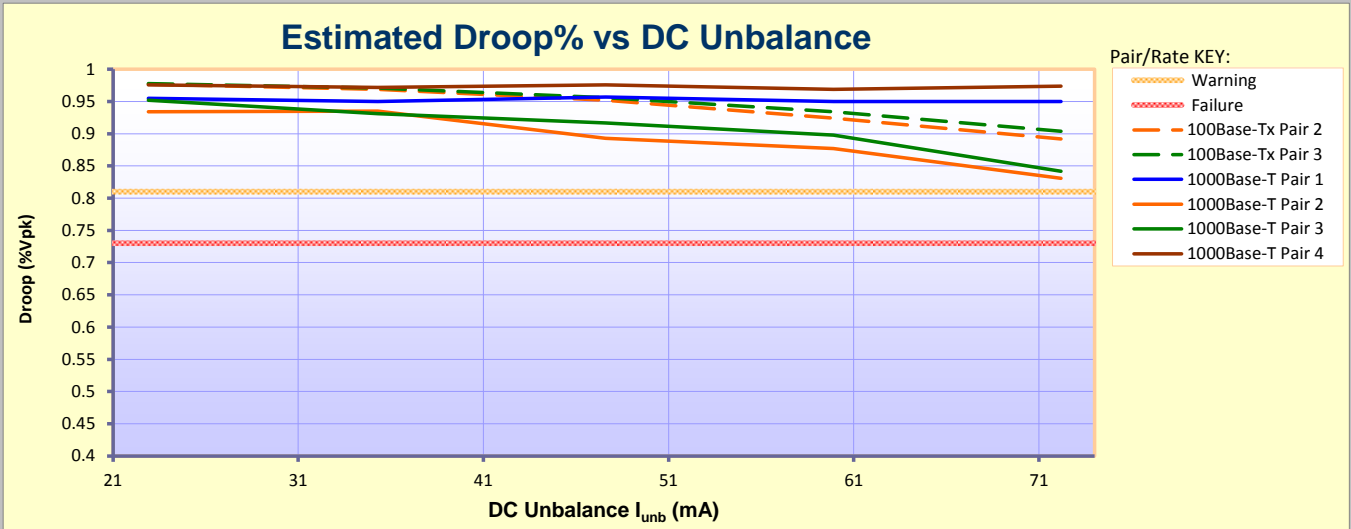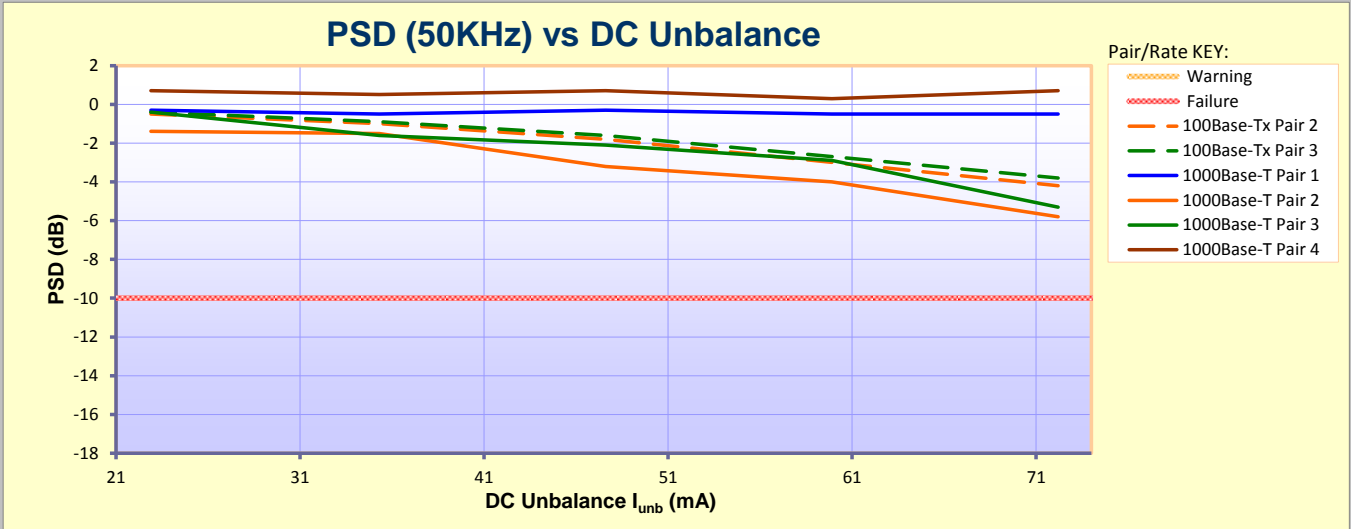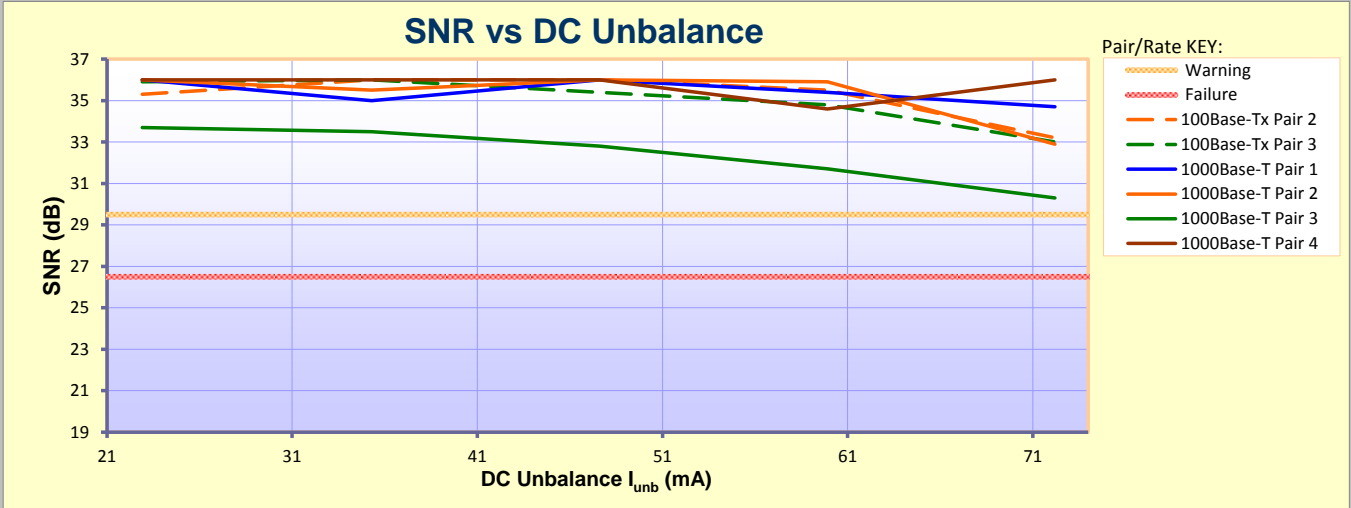

SUMMARY: SNR: Good 50KHz PSD: Good Droop%: Good