

PhyView Analyzer DC Unbalance Report






PVA: 192.168.221.141
PSA: 192.168.221.141

PVA Port: 7-2
PSA Port: 1-2

Date: April 25 2012
Time: 5:45 PM

PSE: Sample Type-2 PSE Port
PSE Port: 1

PHY Suite Version: 4.0.12 04-24-12

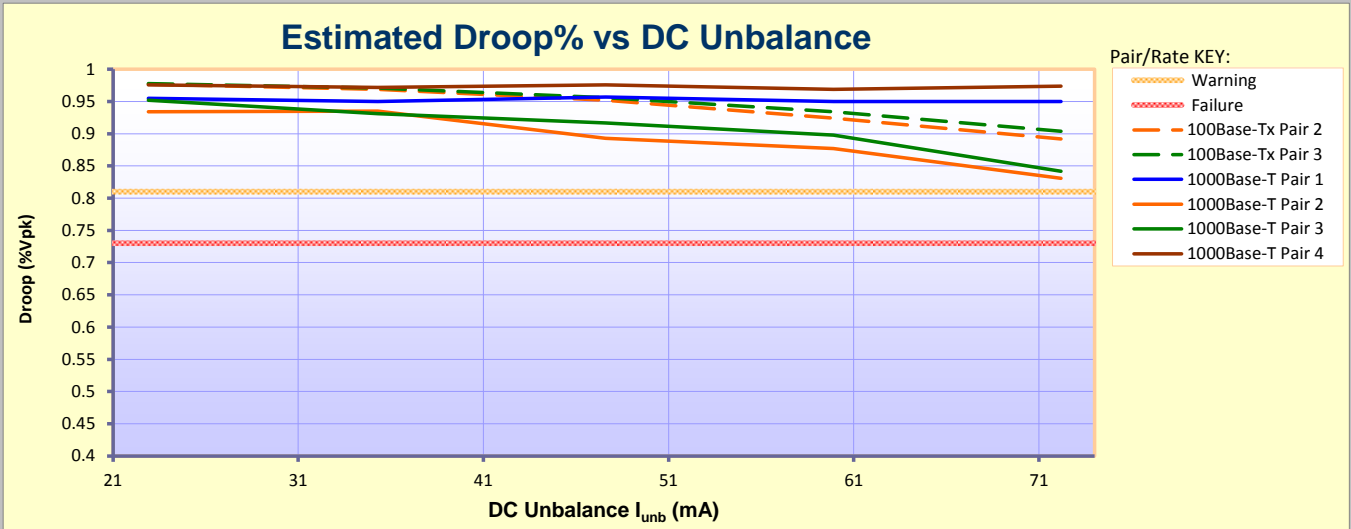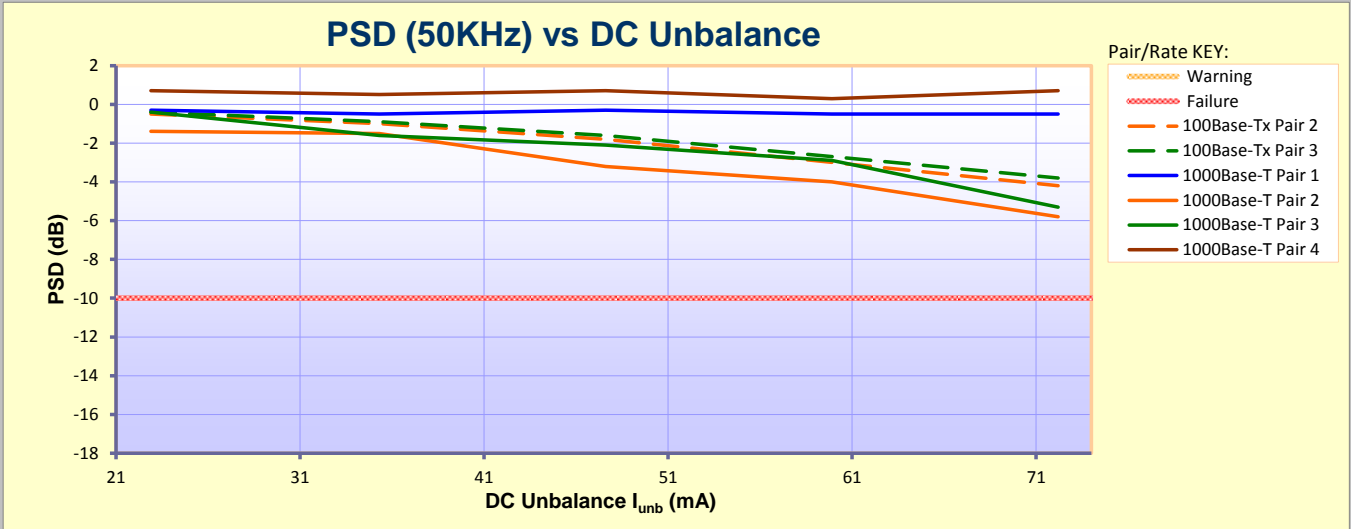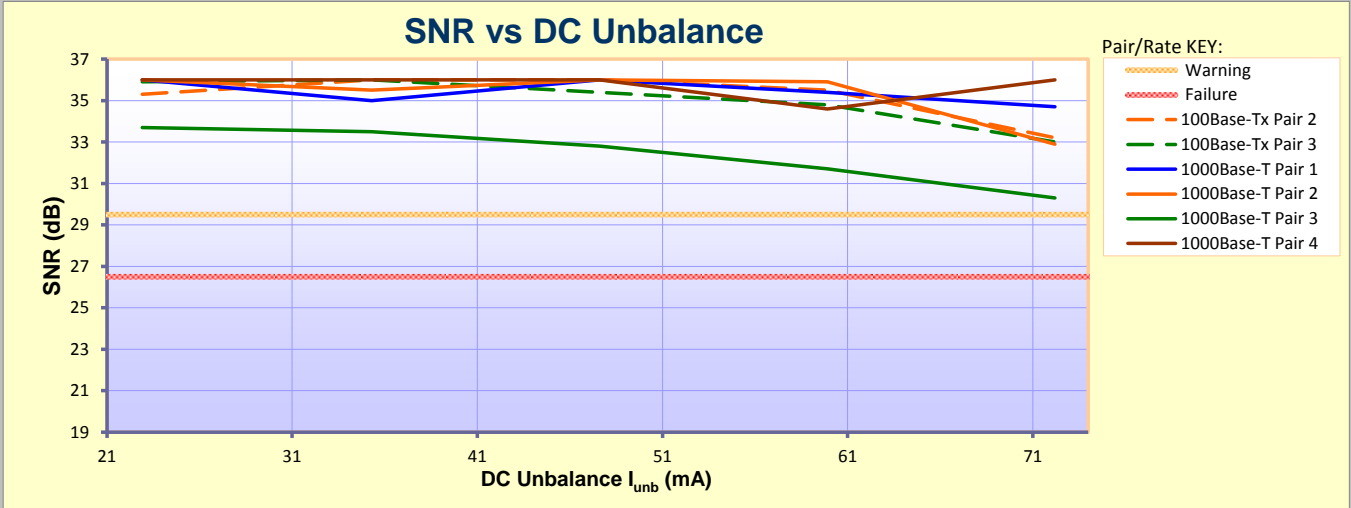

SUMMARY: SNR: Good 50KHz PSD: Good Droop%: Good